



* EN14181 Reporting Facilities *

Calibration function for Raw NO_x

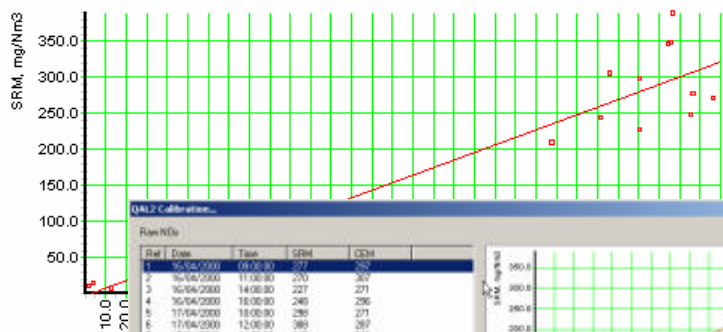


Method(a) Slope
Rsquared: 0.89
Kv=0.9761, Val
C:\mcc\cal\000

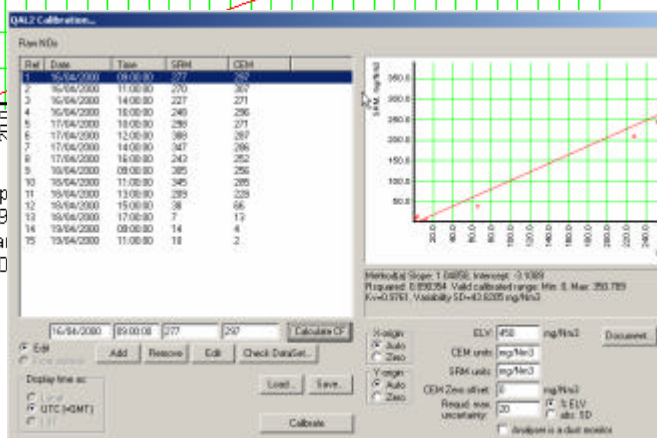

QAL2


Fully automatic

QAL3

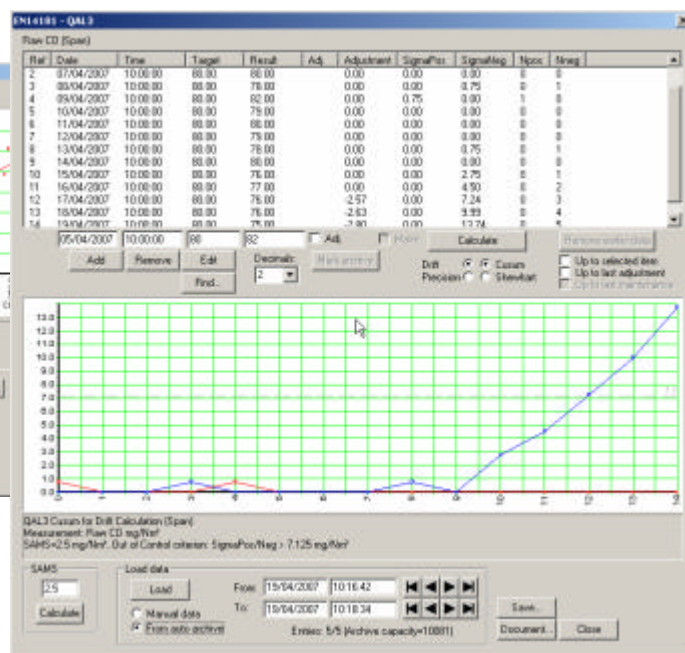

* Auto-E-mailing Utility for immediate action *

Can be activated on any alarm/event, including QAL3 Drift/Precision within percentage of allowable limit:

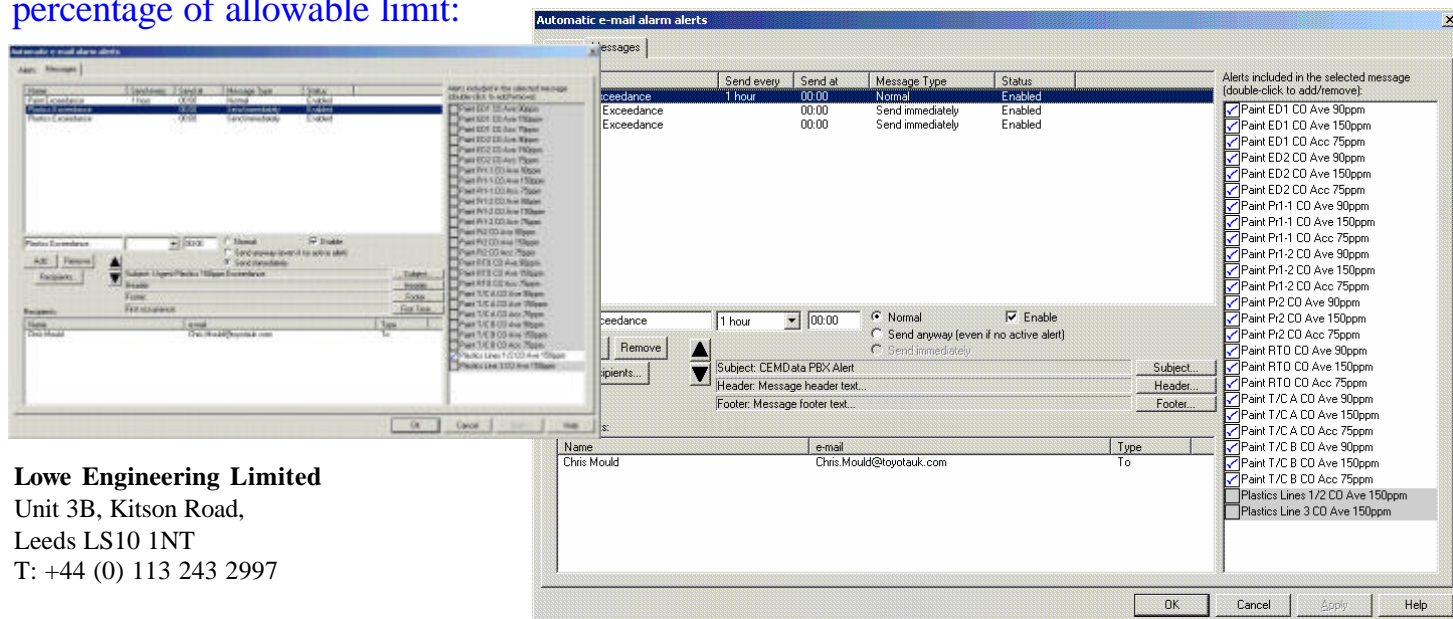

Lowe Engineering Limited
Unit 3B, Kitson Road,
Leeds LS10 1NT
T: +44 (0) 113 243 2997

E: sales@loweengineering.com
W: www.loweengineering.com